
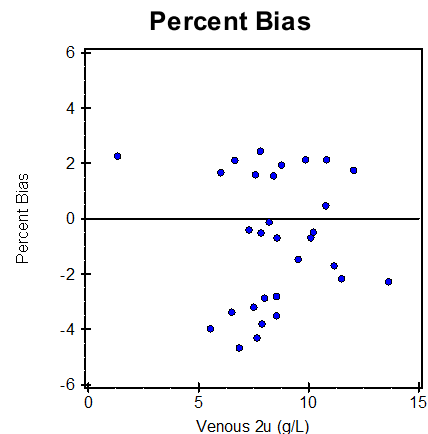
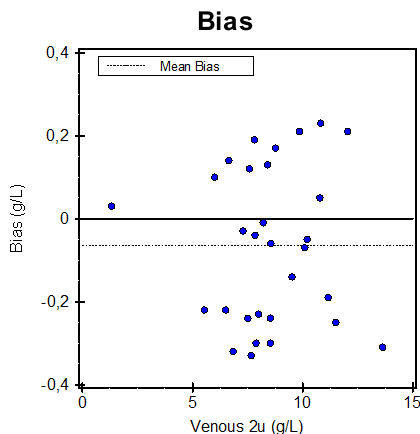


Alternate (Quantitative) Method Comparison

X Method Venous 2u

Y Method Hem-Col 120u

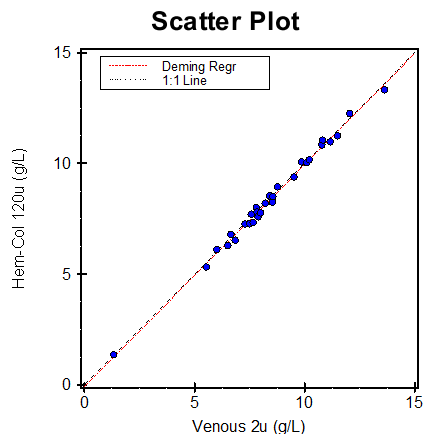

Regression Analysis

	Deming	Regular
Slope	1,004 (0,972 to 1,035)	1,000 (0,969 to 1,032)
Intercept	-0,096 (-0,372 to 0,181)	-0,068 (-0,344 to 0,208)
Std Err Est	0,191	0,191

95% Confidence Intervals are shown in parentheses

Supporting Statistics

Corr Coef (R)	0,9967	SubRange Bounds	None
Bias	-0,066 (-0,772 %)	Points (Plotted/Total)	30/30
X Mean ± SD	8,504 ± 2,320	Outliers	None
Y Mean ± SD	8,438 ± 2,328	Scatter Plot Bounds	None
Std Dev Diff	0,188		

Experiment Description

	X Method	Y Method
Expt Date	13 jun 2018	13 jun 2018
Rep SD	1	1
Result Ranges	1,33 to 13,63	1,36 to 13,32
Units	g/L	g/L
Reagent	--	--
Calibrators	--	--
Analyst	R. Huisman	R. Huisman
Comment		

Accepted by: _____

Signature

Date

Alternate (Quantitative) Method Comparison

X Method Venous 2u

Y Method Hem-Col 120u

Experimental Results




Specimen	X	Y	Bias	Specimen	X	Y	Bias	Specimen	X	Y	Bias
S00001	8,77	8,94	0,17	S00011	6,85	6,53	-0,32	S00021	6,51	6,29	-0,22
S00002	7,29	7,26	-0,03	S00012	11,50	11,25	-0,25	S00022	7,51	7,27	-0,24
S00003	8,54	8,30	-0,24	S00013	12,04	12,25	0,21	S00023	7,89	7,59	-0,30
S00004	6,01	6,11	0,10	S00014	10,82	11,05	0,23	S00024	8,21	8,20	-0,01
S00005	7,81	8,00	0,19	S00015	6,65	6,79	0,14	S00025	11,16	10,97	-0,19
S00006	10,10	10,03	-0,07	S00016	10,78	10,83	0,05	S00026	8,56	8,50	-0,06
S00007	1,33	1,36	0,03	S00017	7,84	7,80	-0,04	S00027	9,52	9,38	-0,14
S00008	8,00	7,77	-0,23	S00018	8,41	8,54	0,13	S00028	7,58	7,70	0,12
S00009	13,63	13,32	-0,31	S00019	10,21	10,16	-0,05	S00029	7,66	7,33	-0,33
S00010	9,86	10,07	0,21	S00020	8,54	8,24	-0,30	S00030	5,54	5,32	-0,22

Values with an "X" were excluded from the calculations. Outliers "O" were also excluded.

Alternate (Quantitative) Method Comparison

X Method Venous 2u

Y Method Hem-Col 120u

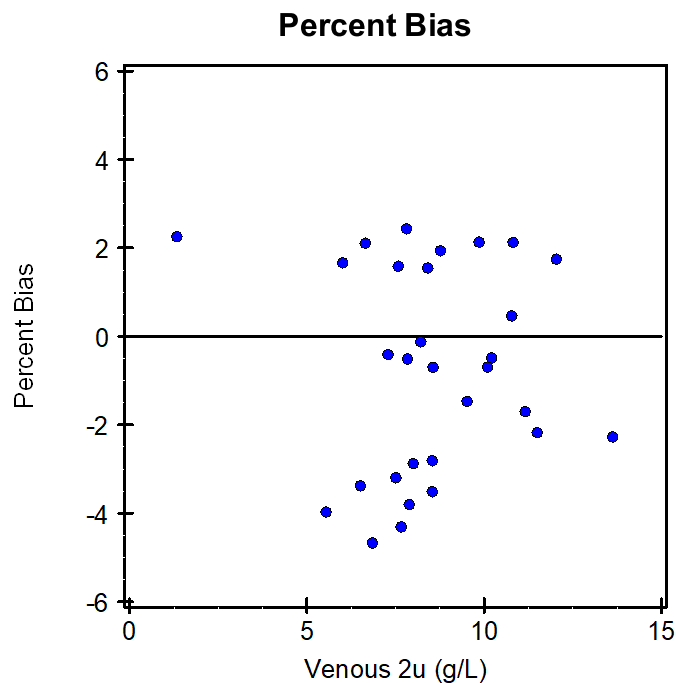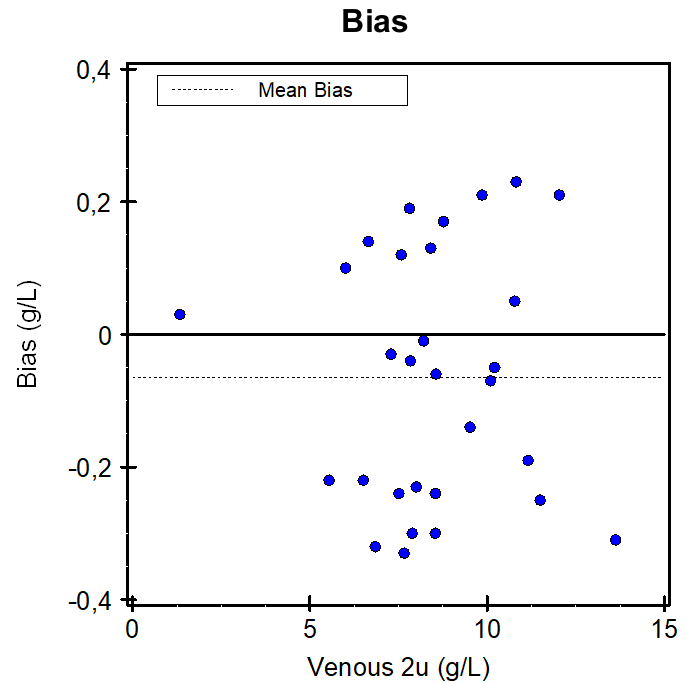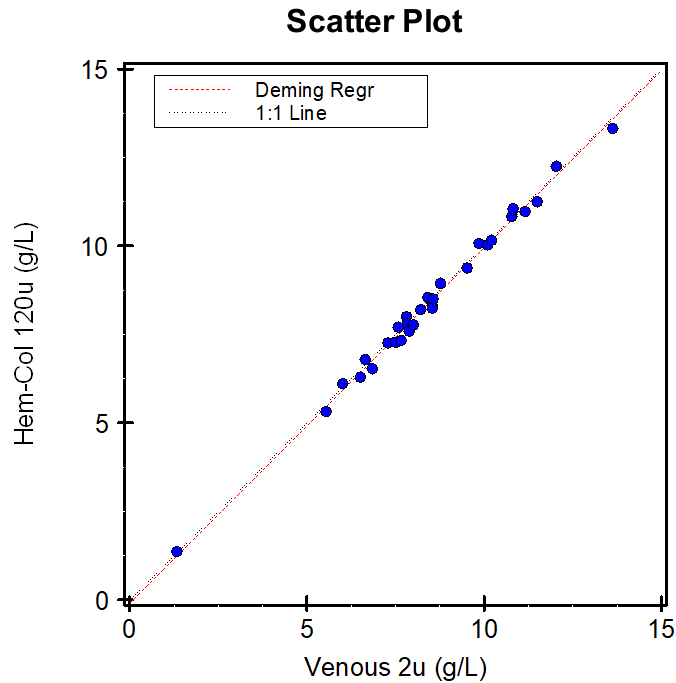

This page contains a larger, working copy of the same graphs that appear on page 1.