


## Alternate (Quantitative) Method Comparison

X Method Venous 2u

Y Method Hem-Col 120u

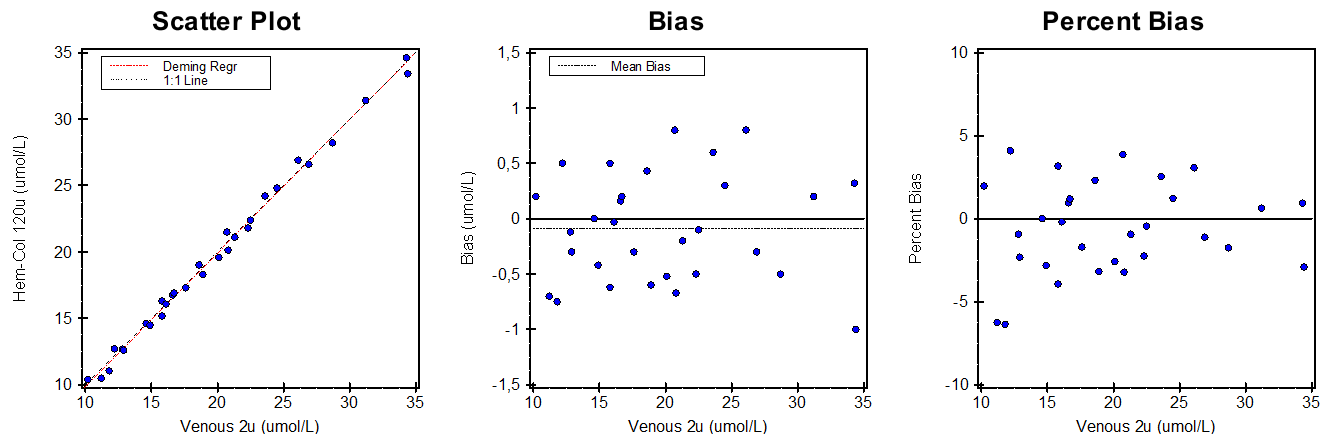

### Regression Analysis

	Deming	Regular
<b>Slope</b>	1,006 (0,977 to 1,034)	1,003 (0,975 to 1,032)
<b>Intercept</b>	-0,202 (-0,796 to 0,392)	-0,148 (-0,742 to 0,445)
<b>Std Err Est</b>	0,499	0,498

95% Confidence Intervals are shown in parentheses

### Supporting Statistics

Corr Coef (R)	0,9973	SubRange Bounds	None
Bias	-0,087 (-0,441 %)	Points (Plotted/Total)	30/30
X Mean ± SD	19,803 ± 6,657	Outliers	Not Tested
Y Mean ± SD	19,716 ± 6,695	Scatter Plot Bounds	None
Std Dev Diffs	0,490		

### Experiment Description

	X Method	Y Method
Expt Date	13 jun 2018	13 jun 2018
Rep SD	1	1
Result Ranges	10,20 to 34,40	10,40 to 34,62
Units	umol/L	umol/L
Reagent	--	--
Calibrators	--	--
Analyst	R. Huisman	R. Huisman
Comment		

Accepted by: \_\_\_\_\_

Signature

Date

### Alternate (Quantitative) Method Comparison

X Method Venous 2u

Y Method Hem-Col 120u

#### Experimental Results




Specimen	X	Y	Bias	Specimen	X	Y	Bias	Specimen	X	Y	Bias
S00001	10,2	10,4	0,2	S00011	23,6	24,2	0,6	S00021	20,10	19,58	-0,52
S00002	14,6	14,6	0,0	S00012	15,8	16,3	0,5	S00022	22,30	21,80	-0,50
S00003	31,2	31,4	0,2	S00013	12,9	12,6	-0,3	S00023	18,60	19,03	0,43
S00004	24,5	24,8	0,3	S00014	16,7	16,9	0,2	S00024	11,80	11,05	-0,75
S00005	26,1	26,9	0,8	S00015	22,5	22,4	-0,1	S00025	14,90	14,48	-0,42
S00006	18,9	18,3	-0,6	S00016	20,7	21,5	0,8	S00026	12,80	12,68	-0,12
S00007	12,2	12,7	0,5	S00017	11,20	10,50	-0,70	S00027	15,80	15,18	-0,62
S00008	34,4	33,4	-1,0	S00018	16,10	16,07	-0,03	S00028	26,90	26,60	-0,30
S00009	17,6	17,3	-0,3	S00019	34,30	34,62	0,32	S00029	28,70	28,20	-0,50
S00010	21,3	21,1	-0,2	S00020	16,60	16,76	0,16	S00030	20,80	20,13	-0,67

Values with an "X" were excluded from the calculations.

### Alternate (Quantitative) Method Comparison

X Method Venous 2u

Y Method Hem-Col 120u

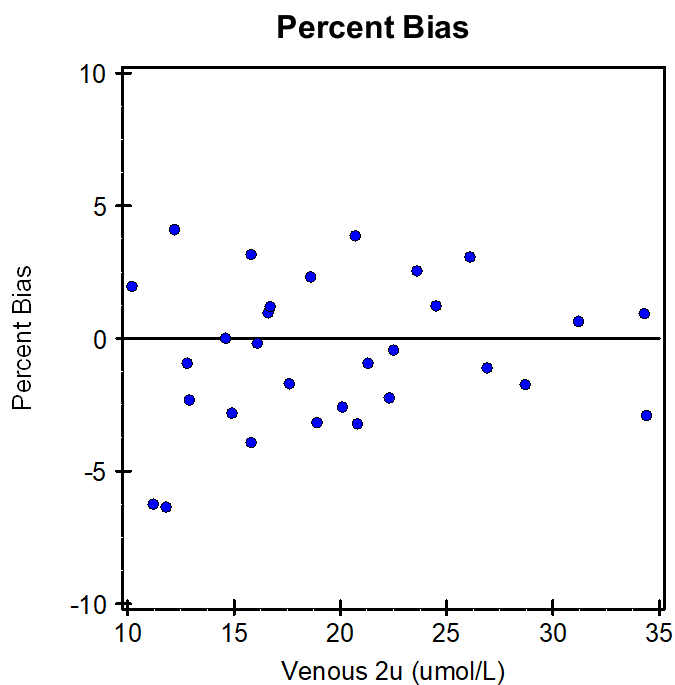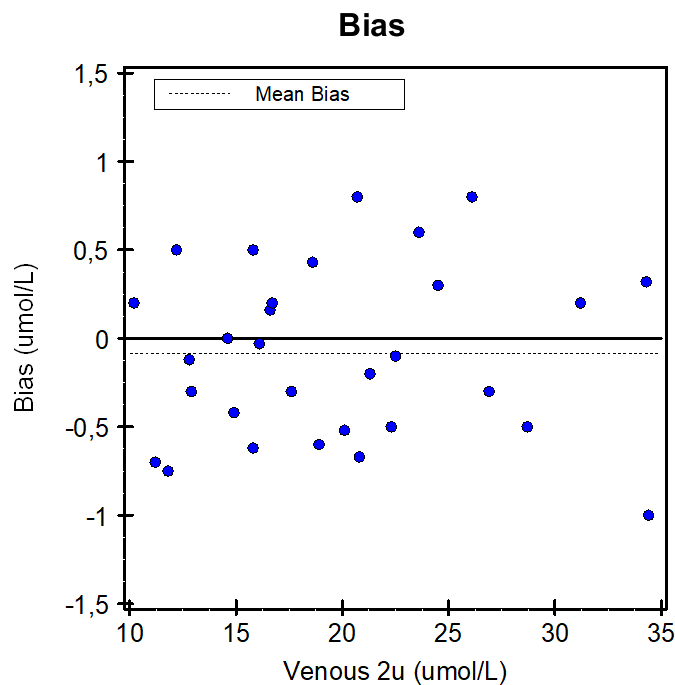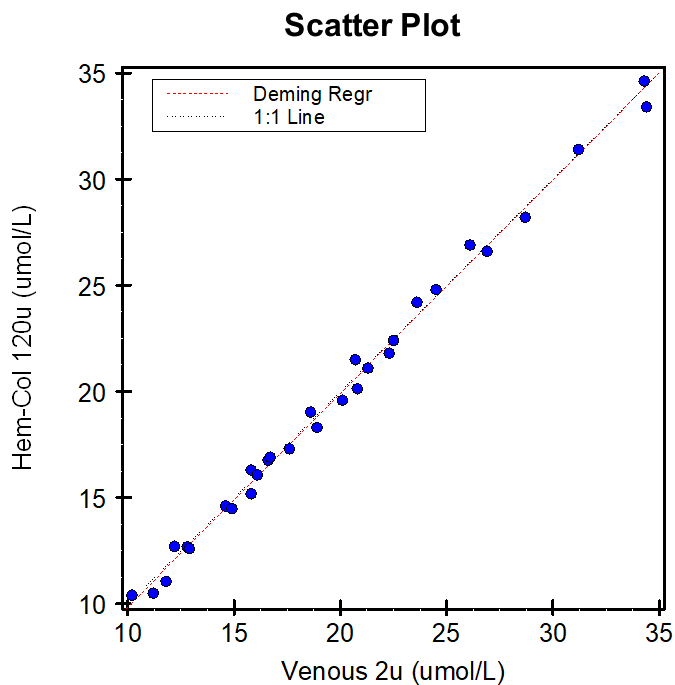

This page contains a larger, working copy of the same graphs that appear on page 1.