


Alternate (Quantitative) Method Comparison

X Method Venous 2u

Y Method Hem-Col 120u

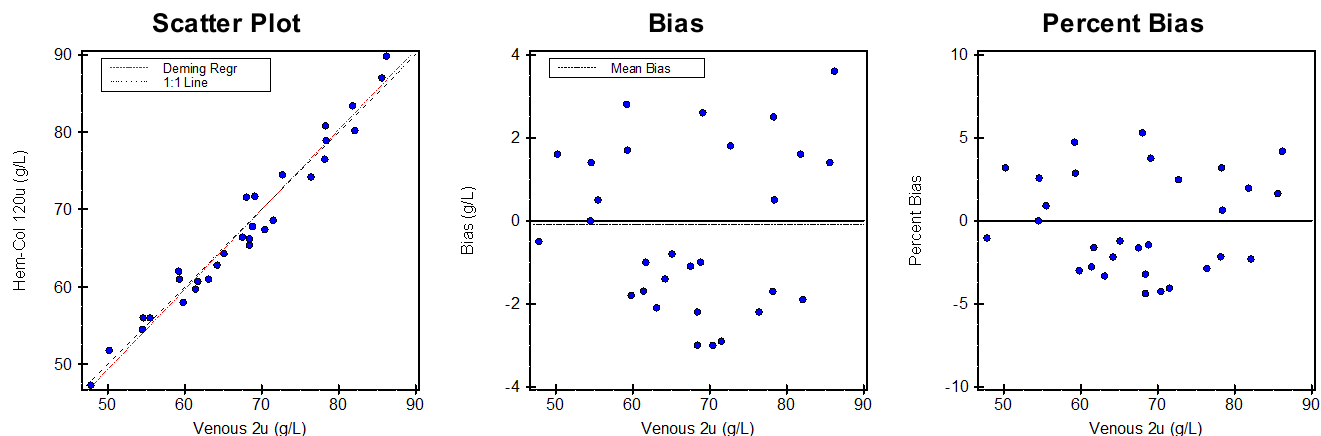

Regression Analysis

	Deming	Regular
Slope	1,033 (0,955 to 1,110)	1,013 (0,936 to 1,090)
Intercept	-2,297 (-7,591 to 2,998)	-0,944 (-6,212 to 4,324)
Std Err Est	2,088	2,078

95% Confidence Intervals are shown in parentheses

Supporting Statistics

Corr Coef (R)	0,9812	SubRange Bounds	None
Bias	-0,090 (-0,133 %)	Points (Plotted/Total)	30/30
X Mean ± SD	67,607 ± 10,256	Outliers	None
Y Mean ± SD	67,517 ± 10,584	Scatter Plot Bounds	None
Std Dev Diff	2,046		

Experiment Description

	X Method	Y Method
Expt Date	13 jun 2018	13 jun 2018
Rep SD	1	1
Result Ranges	47,80 to 86,20	47,30 to 89,80
Units	g/L	g/L
Reagent	--	--
Calibrators	--	--
Analyst	R. Huisman	R. Huisman
Comment		

Accepted by: _____

Signature

Date

Alternate (Quantitative) Method Comparison

X Method Venous 2u

Y Method Hem-Col 120u

Experimental Results




Specimen	X	Y	Bias	Specimen	X	Y	Bias	Specimen	X	Y	Bias
S00001	47,8	47,3	-0,5	S00011	67,5	66,4	-1,1	S00021	76,40	74,2	-2,20
S00002	55,5	56,0	0,5	S00012	81,8	83,4	1,6	S00022	82,10	80,2	-1,90
S00003	68,4	65,4	-3,0	S00013	59,3	61,0	1,7	S00023	54,60	56,0	1,40
S00004	78,4	78,9	0,5	S00014	50,2	51,8	1,6	S00024	63,10	61,0	-2,10
S00005	86,2	89,8	3,6	S00015	69,1	71,7	2,6	S00025	68,80	67,8	-1,00
S00006	70,4	67,4	-3,0	S00016	61,7	60,7	-1,0	S00026	72,70	74,5	1,80
S00007	65,1	64,3	-0,8	S00017	85,60	87,0	1,40	S00027	54,50	54,5	0,00
S00008	61,4	59,7	-1,7	S00018	59,20	62,0	2,80	S00028	59,80	58,0	-1,80
S00009	78,3	80,8	2,5	S00019	64,20	62,8	-1,40	S00029	78,20	76,5	-1,70
S00010	68,0	71,6	3,6	S00020	71,50	68,6	-2,90	S00030	68,40	66,2	-2,20

Values with an "X" were excluded from the calculations. Outliers "O" were also excluded.

Alternate (Quantitative) Method Comparison

X Method Venous 2u

Y Method Hem-Col 120u

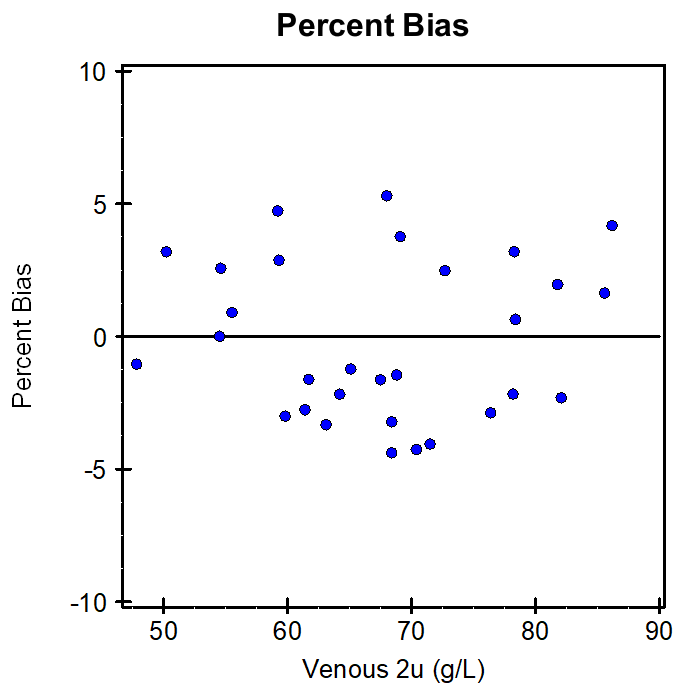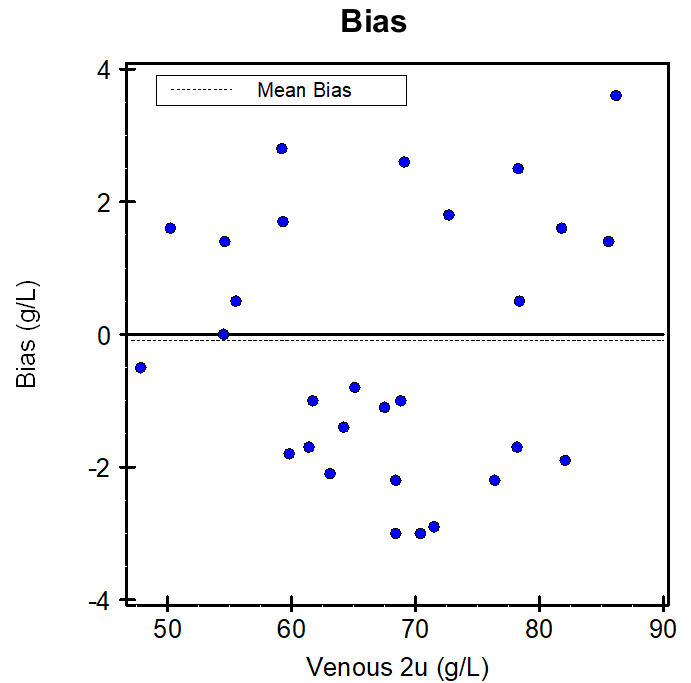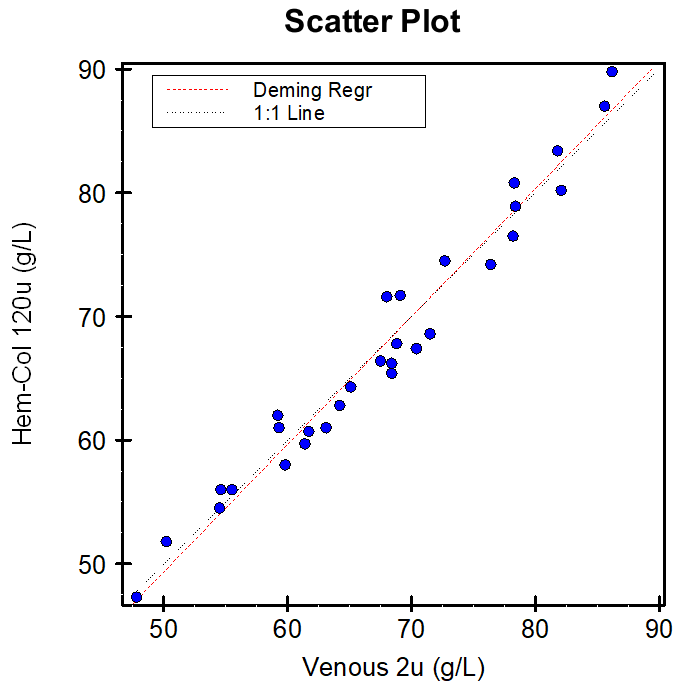

This page contains a larger, working copy of the same graphs that appear on page 1.